

Cadex C5100 Battery Tester



User Guide

Trademark

The Cadex C5100 Battery Tester™ is a registered trademark of Cadex Electronics Inc. All other trademarks or registered trademarks mentioned herein are the property of their respective owners.

Copyright Notice

Copyright © 2009 by Cadex Electronics Inc. All rights reserved. No part of this publication nor the software and/or firmware controlling Cadex product(s) may be reproduced, transmitted, transcribed, stored in a retrieval system, or translated into any language or computer language in any form or by any means without the express written permission of Cadex Electronics Inc.

Revision Rights

Cadex Electronics Inc. reserves the right to revise this publication and make changes in the contents thereof without obligation to notify any person of such changes. Please contact Cadex Electronics Inc. (service@cadex.com) for suggestions or corrections.

Disclaimer

While every effort is made to ensure that the information contained in this manual and Online Help is accurate and up-to-date, Cadex Electronics Inc. does not warrant or guarantee the accuracy of the contents of this manual and Online Help. Further, Cadex makes no warranties, either expressed or implied, as to the merchantability or fitness for a particular purpose of the C5100 Firmware Utility Software or the Cadex C5100 Battery Tester and/or its documentation.

In no event will Cadex or its officers or employees be responsible for any consequential, incidental, or indirect damages (including damages for loss or business profits, business interruption, and the like) arising out of the use or inability to use the Cadex C5100 Firmware Utility Software or the Cadex C5100 Battery Tester and/or its documentation.

Warranty & Service

Cadex Electronics Inc. warrants the Cadex C5100 Battery Tester unit against defective materials and workmanship for one (1) year. Warranty starts from the original date of shipment.

The warranty does not cover:

- Damage caused by abusive operation, negligence, accident, or improper installation.
- Damage caused by an attempted repair not authorized by Cadex.
- Cosmetic damage caused by normal wear and tear.
- Damage from external causes such as leakage spills, power fluctuations, or failure, inadequate packaging.
- If the product is without the appropriate model number, serial number, or safety markings.

- If the product is used for rental purposes.
- Changes or modifications to the equipment not expressly approved by Cadex Electronics Inc.

To obtain service, contact service@cadex.com or (Canada) 1-604-231-7777, (USA Toll Free) 800-565-5228, or (Europe) +49 (0) 911 240 332-0.

Part Number: 89-207-5050

Document Number: PSMAN0070 Rev 1

March 2009

Table of Contents

Section 1: General Precautions and Information.....	5
Safety Notice	5
Use of Equipment	5
Modification of Equipment.....	6
ROHS Compliance	6
Explosion Hazard.....	6
Charging and Discharging Lithium-ion (Li-ion) Batteries	7
Shock Hazard.....	8
Warranty & Service	8
Radio Interference	10
Disposal of Waste Electrical and Electronic Equipment (WEEE) in the European Union...	10
Section 2: Introduction	11
The Cadex C5100 Battery Tester Package	11
Cadex C5100 Battery Tester Features	12
Section 3: Battery Testing	14
Available Programs	14
Test a Li-ion Battery	15
Charge a Li-ion Battery	15
Cycle a Li-ion Battery	16
Select an Active C-Code.....	16
Possible Fault Messages	17
Section 4: Upgrade the C5100 Firmware	18
Upgrade the Firmware	18
Section 5: Maintenance and Spare Components	23
Clean the Battery Adapter or RigidArm Contacts.....	23
Clean the Cadex C5100 Battery Tester	23
Spare Components	24
Section 6: Specifications.....	25

Section 1: General Precautions and Information

Safety Notice

- Read, understand and follow all instructions in this user guide before using the Cadex C5100 Battery Tester unit.
- Refer to the battery manufacturer MSDS (Material Safety Data Sheet) for specific handling and safety information.
- Always inspect a battery for physical damage before testing the battery.

Use of Equipment

The Cadex C5100 Battery Tester is designed with adequate safeguards to protect users from shock and other hazards when used as specified within this document. However, if the equipment is used in a manner not specified by this documentation, the protection provided by this equipment may be impaired. Please read this document and equipment labeling before using the equipment.

Modification of Equipment

CE, FCC, CSA, UL, and other approvals apply only to the Cadex C5100 Battery Tester in the factory-authorized configuration. Changes or modification to the equipment not expressly approved by Cadex will void the approvals.

ROHS Compliance

The C5100 Battery Tester complies with the European Union's Directive 2002/95/EC, Restrictions of Hazardous Substances (RoHS).

Explosion Hazard

Batteries can burst if treated improperly. Follow these precautions at all times:

- ✓ Clean battery contacts before servicing. To clean battery contacts, use a lint-free cotton swab dipped in 100% isopropyl alcohol.
- ✓ Ensure the battery is making a good connection with the adapter contacts.
- ✓ Ensure that the selected C-Code is correct for the chemistry, voltage, and rating of the battery being serviced.
- ✓ Observe battery temperature. Service batteries between 5°C (41°F) and 50°C (122° F). Stop service if battery becomes very hot. The temperatures cited here are the battery temperatures, not the ambient temperatures. Fast charging outside this temperature range may damage or reduce the life of the battery. Allow cold batteries to warm up and hot batteries to cool before charging.
- x Do not attempt to charge non-rechargeable and primary batteries such as alkaline, carbon-zinc, or non-rechargeable lithium batteries.
- x Do not short the positive and negative battery terminals together at any time.
- x Do not exceed the battery manufacturer's recommended charge current and voltage limits for batteries.
- x Do not remove the adapter from the analyzer while the battery is running.

Charging and Discharging Lithium-ion (Li-ion) Batteries

Lithium-ion (Li-ion) batteries are safe when used as directed. Battery safety cannot be assured when a battery pack is built with individual cells of an unknown nature with a series and parallel connection. Not all Li-ion cells are suited for multi-cell packs. Only cells that meet tight voltage and capacity tolerances can be used for series and parallel connection. Mismatched packs are subject to overcharge resulting in venting with flame and fire. Check with the cell manufacturer to see if the cells are suitable for multi-cell packs.

In the past, single Li-ion cells were only available to authorized battery manufacturers. Today, imports are becoming readily available and often fall into the hands of the inexperienced. While most brand name cells are equipped with an internal cell disconnect that permanently opens the current path on high pressure, some brands do not provide this safeguard. Many brands don't use a separator that shuts down the battery when high temperatures are reached. The internal safety features are omitted for cost reasons.

Please follow the following guidelines when charging and discharging lithium-ion cell(s) and packs. Failing to follow these rules could result in venting with flame, explosions, fire, and personal injury.

- x Never connect cells in parallel and/or series that are not designed for that purpose. A cell mismatch may overcharge and vent with flames
- x Never charge or discharge the battery without connecting a working protection circuit. Each cell must be monitored individually and the current disconnected if an anomaly occurs.
- x Never leave the battery unattended while under charge or discharge.
- ✓ Always attach a temperature sensor when charging and discharging the battery. The temperature sensor must disconnect the current on excess temperature.
- ✓ Only connect cells that are matched and have the identical state-of-charge.

- ✓ Pay special attention when using an unknown brand. Not all brands contain intrinsic safety features that protect the cell when stressed.
- ✓ During experiments, place the test battery into a well-ventilated fireproof container.

Shock Hazard

The Cadex C5100 Battery Tester contains high-voltage circuits, and can pose a shock hazard when the unit is opened. Do not attempt to open the unit - there are no user-serviceable items inside.

- ✓ To reduce the risk of electrical shock hazard, service batteries only when they are removed and disconnected from their end-use equipment.
- ✓ Use the tester only as specified in the documentation. Other uses may impair the protection provided by the unit.
- ✓ Use only a grounded AC outlet to power the tester.

Warranty & Service

Cadex Electronics Inc. warrants the Cadex C5100 Battery Tester against defective materials and workmanship for a period of one (1) year from the original purchase date.

The warranty does not cover:

- Damage caused by abusive operation, negligence, accident, or improper installation.
- Damage caused by an attempted repair not authorized by Cadex.
- Cosmetic damage caused by normal wear and tear.
- Damage from external causes such as leakage spills, power fluctuations, power failure, or inadequate shipping.
- Products received without the appropriate model number, serial number, or safety markings.
- Products used for rental purposes.

Warranty Service

Before sending the unit for service, contact Cadex Technical Support at (Canada) 1-604-231-7777, (USA Toll Free) 800-565-5228, or (Europe) +49 (0) 911 240 332-0 or service@cadex.com. If the product requires warranty service, the representative will provide a Return Authorization form or number and the location of the nearest service center.

- Ship the product to the service center with freight, insurance, and customs duties prepaid. The Return Authorization form must be included to obtain warranty service.
- Ensure that the unit(s) is properly packed before shipping, preferably in the original Cadex boxes. Damage caused in transit due to improperly packed items is not covered under warranty.
- Products returned from warranty service are shipped with freight prepaid by Cadex.

Non-Warranty Repairs

Before sending the unit in for service, contact Cadex Technical Support at (Canada) 1-604-231-7777, (USA Toll Free) 800-565-5228, or (Europe) +49 (0) 911 240 332-0, or service@cadex.com. If the tester is not covered by warranty, the representative will provide the contact information for the nearest service center. Contact the service center directly to arrange to send the product in for service. A Return Authorization form or number will be provided only if the product is returning to the Cadex Head Office.

- Ship the product to the service center with freight, insurance, and custom duties prepaid.
- Ensure that the unit(s) is properly packaged before shipping.

Note: Cadex Electronics Inc. and Cadex authorized service centers require a Purchase Order or written authorization to proceed with repairs.

Radio Interference



This equipment generates, uses, and radiates radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause interference with radio communications. It has been tested and found to comply with the limits for a Class “A” digital device pursuant to Subpart B of Part 15 of the FCC Rules, which are designed to provide reasonable protection against such interference when operated in a commercial environment. Operation of this equipment in a residential area may cause interference, in which case the user, at their expense, is required to take whatever measures needed to correct the interference.

EN55022 Warning: This is a Class A product according to EN55022. In a domestic environment, this product may cause radio interference, in which case the user, at their own expense, may be required to take adequate corrective measures.

The equipment is designed with adequate safeguards to protect the user from shock and other hazards when used as specified within this document. If the equipment is used in a manner not specified by the documentation, the protection provided by the equipment may be impaired. Please read the documentation and equipment labeling before using the equipment.

Disposal of Waste Electrical and Electronic Equipment (WEEE) in the European Union



This symbol on the product and package indicates that this product must not be disposed with unsorted municipal waste. Instead, it is your responsibility to dispose of WEEE by handing it over to a designated collection point for the disposal. The separate collection and recycling of waste equipment will help conserve natural resources and ensure that it is disposed in a manner that protects human health and the environment. For more information about where you can drop off your waste equipment for disposal, please contact your local municipal office, waste disposal service or where you purchased the product.

Section 2: Introduction

The Cadex C5100 Battery Tester is a tester and charger for Li-ion type batteries. The C5100 uses sophisticated algorithms to determine the current state of the battery.

The Cadex C5100 Battery Tester Package

The Cadex C5100 Battery Tester package contains the following items:

- Cadex C5100 Battery Tester unit.
- RigidArm Universal Battery Adapter.
- Country-specific AC power cord.
- This user guide.



IMPORTANT NOTICE

Use only grounded AC power cord(s) and outlets with the Cadex C5100 Battery Tester.

Cadex C5100 Battery Tester Features

The LCD backlight on the Cadex C5100 Battery Tester automatically turns off after five minutes of inactivity. The LCD backlight will turn itself on when any key is pressed on the unit or when the running program is completed.

The front panel of the Cadex C5100 Battery Tester has three LEDs: Run (yellow), Ready (green), and Fail (red). The front panel also contains three buttons (Test, Charge, and Cycle) and two scroll buttons.



Test	Performs battery rapid test using Cadex QuickSort™. Classifies batteries into three ranges – Good, Low, or Poor. Approximately 30 seconds.
Charge	To charge a battery. Approximately 3 hrs.
Cycle	Cycles a battery with charge/discharge/charge and displays measured capacity as a % of the C-Code rated value. Approximately 7 hrs.
Directional keys	To scroll through menus and results.
Main Display	LCD viewing panel
LEDs	LED status indicators



- | | |
|----------------|--|
| Serial port | To connect to a computer. Cable not included. |
| AC Power Inlet | Attach AC power cord to IEC320 inlet. |
| USB Port | To connect to a USB port for a firmware upgrade. Type B USB connector. Requires a Type A to Type B USB cable for connecting to a PC. Cable not included. |

Section 3: Battery Testing

Available Programs

The **Boost** program reactivates batteries that fall asleep due to over-discharge and brings the battery back to life. The program charges the battery for two minutes at 100mA.

The **Test** program performs battery rapid test using Cadex QuickSort™ with consideration for the parameters of the selected C-Code and classifies the status of the battery as Good, Low, or Poor within 30 seconds. The range is 3.6V Li-ion 500-1500mAh. Batteries outside this range will not be tested and a message *No QuickSort Support* appears.

The **Charge** program charges the battery based on the parameters in the selected C-Code in about 3 hours.

The **Cycle** program performs charge/discharge/charge on the battery based on the parameters in the selected C-Code, and displays measured capacity as a % of the C-Code rated value in approximately 7 hours.

Note: If a battery C-Code that is not supported by the C5100 is selected, the unit will display one of these messages: *NiCd Not Supported*, *NiMH Not Supported*, *SLA Not Supported*, *10.80V Not Supported*, or *14.40V Not Supported*.

Boost Program

Applies 100mA Charge for Two Minutes

1. Apply AC power to turn on the Cadex C5100 Battery Tester. The Run LED light will flash if a battery adapter is installed and a battery is inserted in the adapter.
2. Insert the Li-ion battery to boost.
3. Hold down any program key (Charge, Test, or Cycle) for two seconds. The C5100 will display *Caution Boosting, Press ▼ to Esc, Check Polarity*, and then *Press ▲ to Continue*.
4. If the ▲ key is pressed, it will display *Press Program key for 2 seconds*.
5. Press and hold a program key (Charge, Test, or Cycle) for 2 seconds to activate the **Boost** program.
6. **Boost** can be cancelled anytime by pressing the down arrow key.

Test a Li-ion Battery

Rapidly Test the Battery Condition in Less Than 30 Seconds

1. Apply AC power to turn on the Cadex C5100 Battery Tester. The Run LED light will flash if a battery adapter is installed and a battery is inserted in the adapter.
2. Insert the Li-ion battery to test.
3. Select the correct C-Code for the battery by pressing the ▼▲ keys.
4. Press **Test**. The battery test begins.
5. When the battery test is completed, the test results appear on the screen.

If a battery is faulty or is determined to be in poor condition, the Fail LED light will be turned on and the display will indicate the battery's condition, as follows:

Good Battery: A battery that does not have any of the following: shorted, open cells, above normal impedance; and which residual capacity is higher than 80% of its rated value, based on the selected C-Code.

Poor Battery: A battery that has any of the following: shorted, open cells, above normal impedance, 70% or less residual capacity compared to its rated value, based on the selected C-Code.

Low Battery: A battery that does not have any of the following: shorted, open cells, above normal impedance; and which residual capacity is between 70% and 80% of its rated value, based on the selected C-Code.

Charge a Li-ion Battery

A battery is charged in about three hours.

1. Apply AC power to turn on the Cadex C5100 Battery Tester. The Run LED light will flash if a battery adapter is installed and a battery is inserted in the adapter.
2. Insert the Li-ion battery to charge.

3. Select the correct matrix for the battery by pressing the ▼ or ▲ key.
4. Press **Charge**. The C5100 will perform a fast charge.
5. When the battery has finished charging, the Ready LED will be lit. If there was a problem during charge, the Fail LED will be lit.

Cycle a Li-ion Battery

The Cycle button charges/discharges/charges a battery and displays the battery's capacity in % in about 7 hours.

1. Apply AC power to turn on the Cadex C5100 Battery Tester. The Run LED light will flash if a battery adapter is installed and a battery is inserted in the adapter.
2. Insert the Li-ion battery to cycle.
3. Select the correct matrix for the battery by pressing the ▼ or ▲ key.
4. Press **Cycle**. The C5100 will perform charge/discharge/charge and indicate the measured capacity result in %.
5. When the battery has finished cycling, the Ready LED will be lit and the battery's capacity in % indicated on the display. If there was a problem during cycling, the Fail LED will be lit.

Select an Active C-Code

The Cadex C5100 Battery Tester uses one C-Code of the available C-Codes (10 maximum) stored in the installed battery adapter as the active C-Code.

To select a different active C-Code:

1. Insert a Li-ion battery. Press the ▼▲ keys to select the appropriate C-Code.
2. Press the appropriate program button to start processing.

The battery Voltage and C-Code rated Capacity (mAh) are displayed for each C-Code.

Possible Fault Messages

Contact Cadex Technical Support at (Canada) 1-604-231-7777, (USA Toll Free) 800-565-5228, or (Europe) +49 (0) 911 240 332-0, or service@cadex.com for further information.

'VREF OUT OF RANGE, MAY NEED CALIBRATION'

'VREF OUT OF RANGE, SERVICE REQUIRED'

'ERROR: %5i'

'ERROR: CLEARED'

'BAD FUSE OR DRIVER'

'OVERCURRENT BREAK'

Section 4: Upgrade the C5100 Firmware

Upgrade the Firmware

To upgrade the **C5100 Firmware** requires using the **Cadex C5100 Firmware Utility**. Contact Cadex Customer Service at (Canada) 1-604-231-7777, (USA Toll Free) 800-565-5228, or (Europe) +49 (0) 911 240 332-0, or service@cadex.com to obtain the C5100 Firmware Utility and the C5100 Firmware. Next, follow these instructions to upgrade the C5100 firmware utility.


The **Cadex C5100 Firmware Utility** can update the C5100's firmware. A USB type A to type B cable is required to connect the C5100 to the PC's USB port (cable not included).

To update the firmware on the C5100:


1. The contents of the ZIP may need to be extracted from the ZIP file to a new folder. The **About Cadex C5100 Firmware Utility** window appears.




2. Click **OK** to continue. The **Select a C5100 firmware file** window appears.

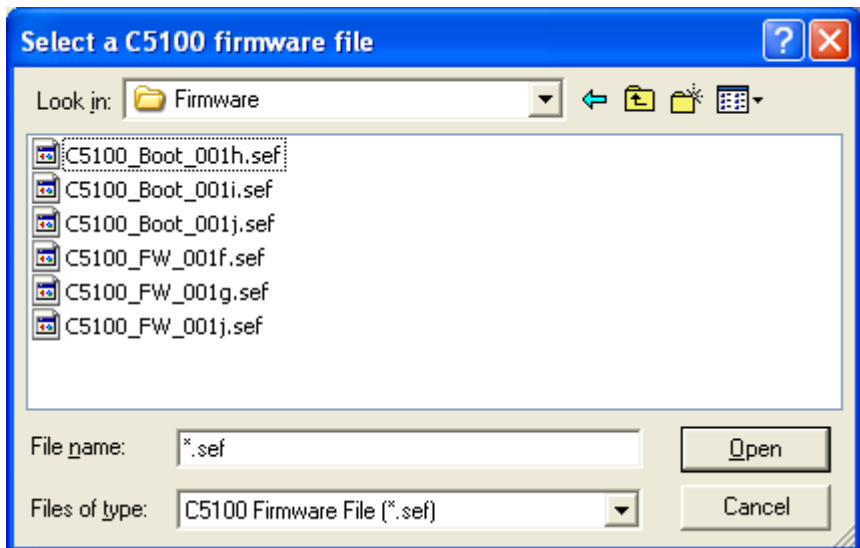

3. Select the appropriate firmware file and click **Open**. The **Firmware Update** window appears.

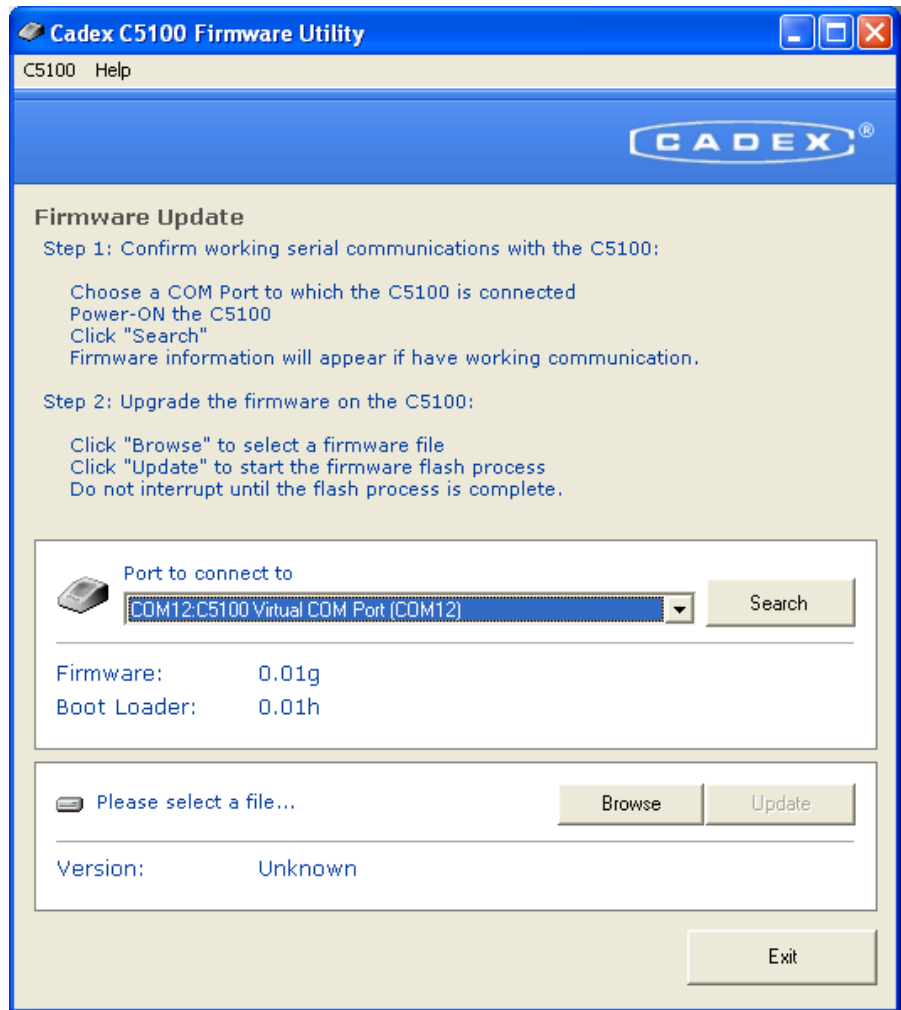

4. Click the DOWN ARROW in the *Port to connect to* field to select the COM port that the C5100 is connected to. Ensure AC power is applied to the C5100 and the USB type A to type B cable (not included) is connected from the C5100 (type B) to one of the PC's USB ports (type A). Click **Search**. If there is a working connection, the firmware information appears.
5. Click **Browse** to select a firmware file. Next, click **Update** to initiate the firmware flash process. The **Confirm** window appears.




Note: The **Confirm** window may ask if you want to downgrade the firmware. If so, click **OK**.




6. Click **Browse** to select a firmware file. Next, click **Update** to initiate the firmware flash process. The **Confirm** window appears.
7. Click **Yes** to update the firmware.



8. The **Information** window appears when the firmware has been updated.



9. Click **Exit**. The **Confirm** window appears. Click **Yes** to exit the firmware utility.



10. The **Information** window appears. Disconnect the USB cable from the C5100 and click **OK**.



If error messages occur, contact Cadex Technical Support at (Canada) 1-604-231-7777, (USA Toll Free) 800-565-5228, or (Europe) +49 (0) 911 240 332-0, or service@cadex.com.

Section 5: Maintenance and Spare Components

To maintain accuracy in test results and long life, Cadex Electronics Inc. recommends the following steps to maintain the C5100.

Clean the Battery Adapter or RigidArm Contacts

Clean the battery adapter contacts regularly with a lint free cotton swab and isopropyl alcohol. This will ensure that the readings are accurate.

Clean the Cadex C5100 Battery Tester

1. Do not use any cleaning solution on the C5100 unit.
2. Wipe the unit with a clean damp cloth.

Spare Components

The following replacement parts may be purchased from Cadex Electronics Inc. Please contact service@cadex.com for pricing and delivery.

Description	Part Number
IEC320 6' UK Plug AC Power Cord	68-723-1805
IEC320 6' Euro Plug AC Power Cord	68-723-1806
IEC320 6' North American AC Power Cord	68-723-1810
PC to C5100 RS-232 Cable	68-940-0006
RigidArm Universal Battery Adapter	07-110-0190
USB Type A to Type B Cable	68-931-0008

Cadex offers over 1,000 custom Battery Adapters to accommodate most batteries. These adapters are factory programmed and will configure the C5100 for the correct battery parameters. Please check the battery adapter catalog at:
http://www.cadex.com/prod_analyzers/adapters.asp.

Section 6: Specifications

Application: Single-station standalone battery tester.

Range: Supports 3.6V or 7.2V Li-ion batteries, user-selectable. Test program only supports 3.6V Li-ion, 500-1500mAh batteries, user-selectable.

Charge/discharge: 2A max.

Battery Interface: Custom and universal adapters; Cadex SnapLock™ system; read-only application, temperature sensor.

Line voltages: 100-240VAC, 50/60Hz 0.6A, internal power supply, IEC320 grounded inlet, country-specific AC power cords available.

Programs: 3 buttons, up/down selection keys

Test 30s QuickSort™ test

Charge 3h fast charge

Cycle Charge/discharge/charge

Boost Reactivates batteries that have fallen asleep due to low discharge

Display: LCD screen 2X20, backlit; RUN, READY, FAIL light signals.

Data Ports: USB Type B, RS232 9 pin female DSUB for firmware upgrade.

Physical: H 92; W 160; L 285mm (3.6x 6.3x11.2"); 0.82kg net (1.8lb)

Approvals: CSA/UL/EN60950, CE marked, ROHS and WEEE.

Warranty: One (1) year for materials and workmanship.

Note: Specifications subject to change without notice.